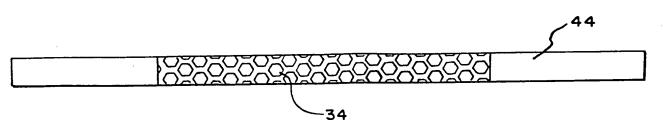
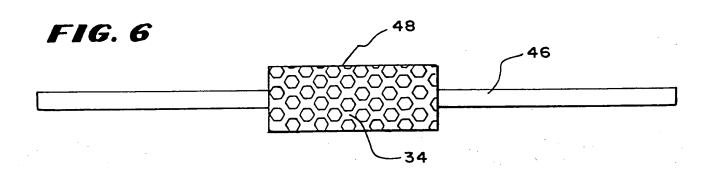
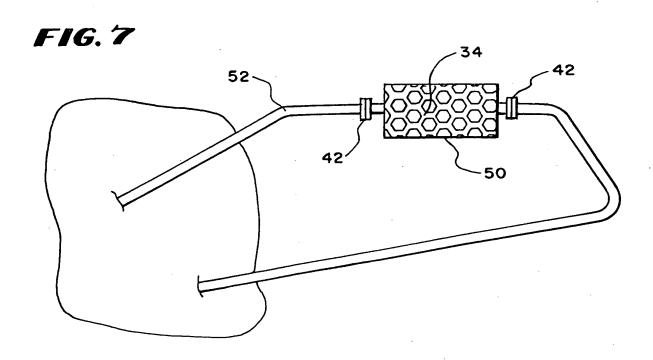
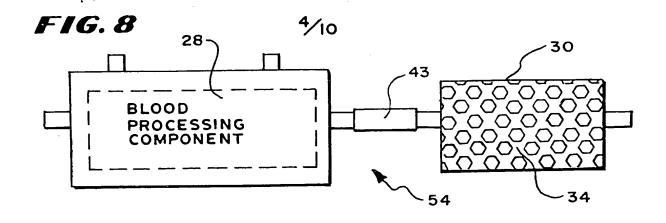



FIG. 5











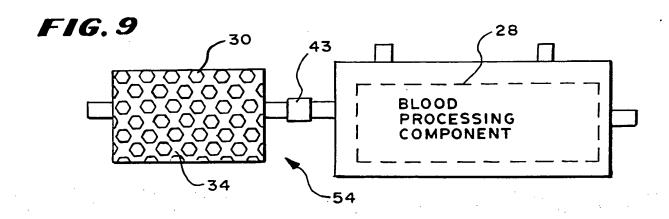

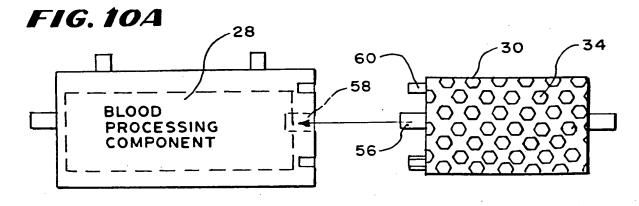

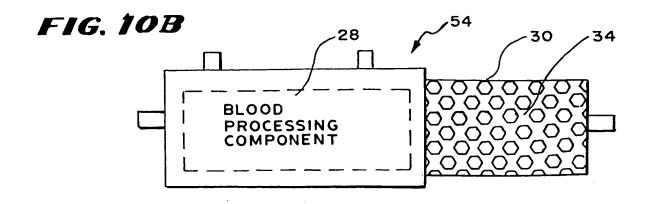

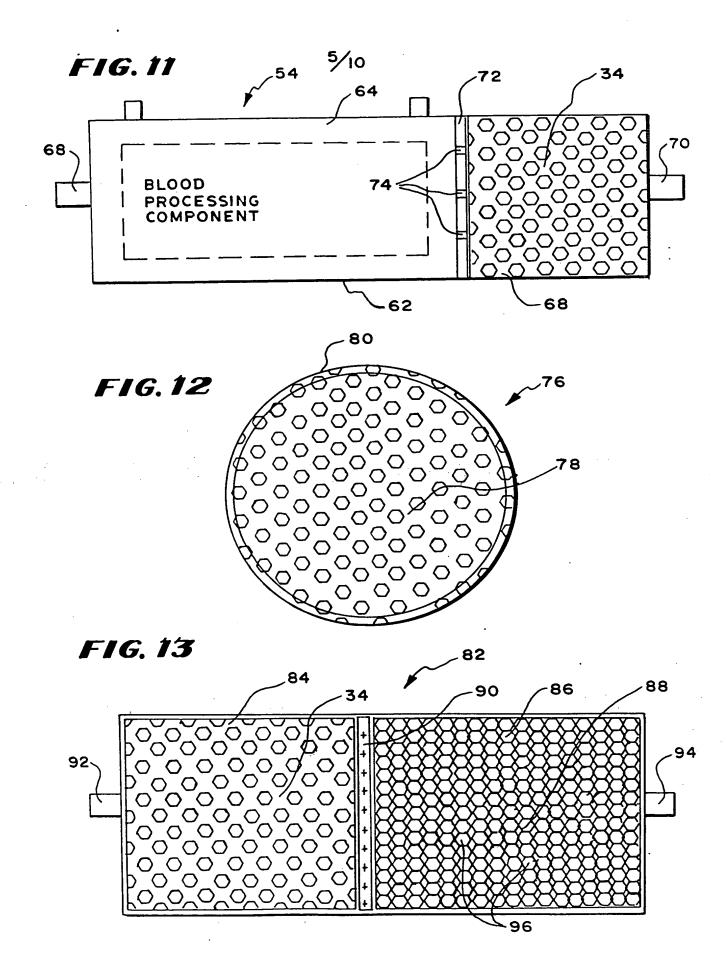


FIG. 14


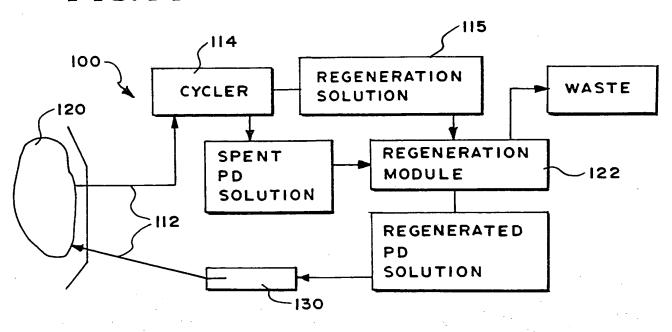


FIG. 15

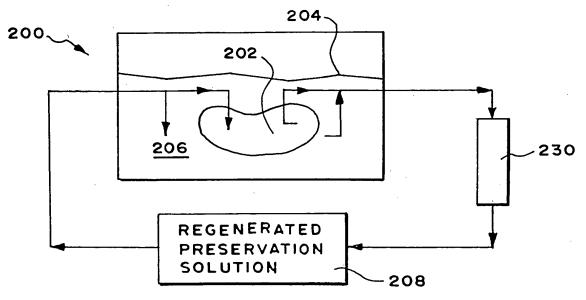

P1(I0 mL/min)

P3(2 mL/min)

300

P1(I0 mL/min)

304

304

314

SAMPLE

SAMPLE

FIG. 17

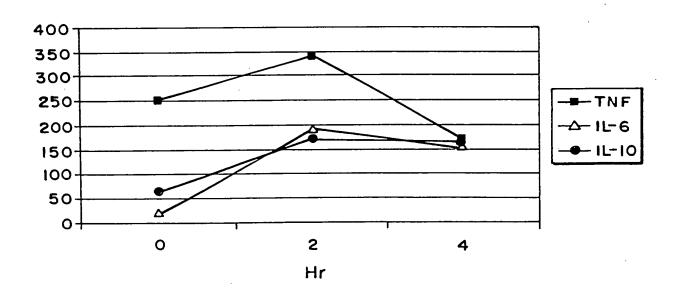


FIG. 18A

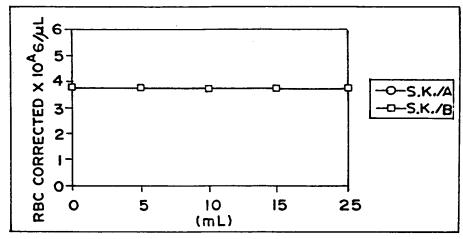


FIG. 18B

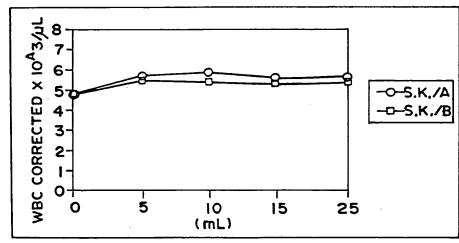


FIG. 18C

